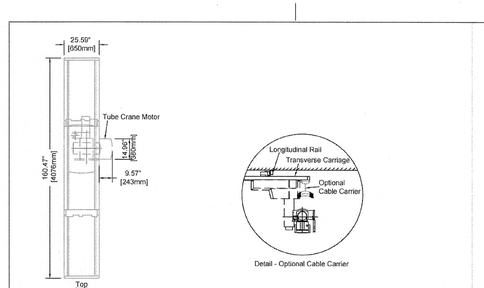

* Column movement range = 2890mm (117.32"); standard range of 3190mm reduced by 210mm (8.28") to allow optional cable carrier to be mounted on transverse carriage.

Optional cable carrier can be mounted on longitudinal rail, causing 210mm (8.28") of tube crane coverage loss at foot- or head-end.

(09.0)

MU	CS 4 Tube Crane	
Weight	922 lbs	(419 kg)
Heat Dissipation	1297 Btu/hr	(326 kcal/hr)

* Extension Rails are an additional 113lbs (51kg).

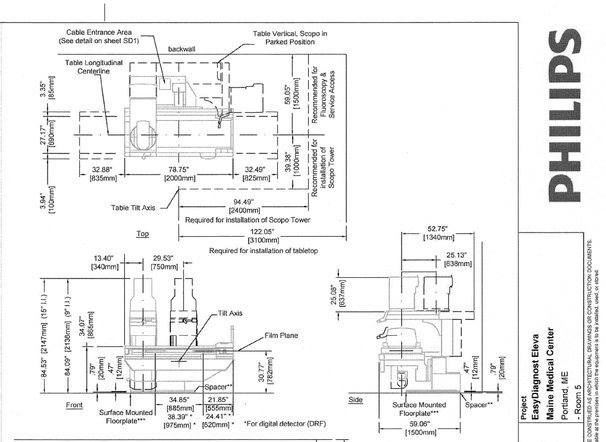

Minimum Ceiling Height: 2720mm (8'-11")
Maximum Ceiling Height: 3110mm (10'-2 9/16")

Recommended ceiling height of (10'-4") allows tabletop to clear ceiling rails when fully extended vertically.

**Spacer thickness: 12mm (½")
***Floorplate thickness: 20mm (13/16")

(09.0)

MS	Easy Diagnost Eleva	
Weight	3044 lbs	(1381 kg)
Heat Dissipation	2047 Btu/hr	(516 kcal/hr)

PHILIPS

Project
EasyDiagnost Eleva
Maine Medical Center
Portland, ME
- Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number:207-451-0546
Email: wayne.erwin@philips.com
Drawn By: JP Ganzhalian

Project Details
Drawing Number
N-EAS1006I12A
Date Drawn: 6/21/2010
Quote:1-PST1JCL Rev.7
Order:6900069926.001000

AD1

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or the utilities available at the premises on which the equipment is to be installed, used, or stored.

© Koninklijke Philips Electronics N.V. 2008. All rights reserved. Reproduction in whole or in part is prohibited without prior written consent of the copyright holder.

THIS SHEET IS PART OF THE DOCUMENT SET LISTED ON SHEET C1 AND SHOULD NOT BE SEPARATED.



(09.0)

BVS	Bucky Diagnost VS Advanced	
Weight	439 lbs	(198 kg)
Heat Dissipation	546 Btu/hr	(138 kcal/hr)

Weight of wall connection box: 22 lbs. (10 kg.)



(06.0)

IR	Infra Red Receiver	
Weight	1 lbs	(0.45 kg)
Heat Dissipation	3 Btu/hr	(0.76 kcal/hr)



(09.0)

IB	Indication Box	
Weight	2lbs	(1 kg)
Heat Dissipation	34 Btu/hr	(9 kcal/hr)



(09.0)

QR	Quick Review	
Weight	3 lbs	(1 kg)
Heat Dissipation	7 Btu/hr	(2 kcal/hr)

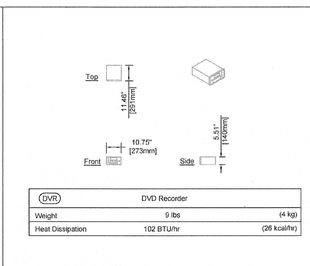

DVR	DVD Recorder	
Weight	9 lbs	(4 kg)
Heat Dissipation	102 BTU/hr	(26 kcal/hr)



CPU Tower
Weight: 32 lbs (15kg)
Heat Dissipation: 293 btu/hr (73 kCal/hr)

Eleva Examination Control Economy
Weight: 19 lbs (9kg)
Heat Dissipation: 342 btu/hr (86 kCal/hr)

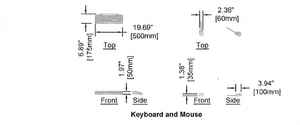

Keyboard and Mouse

(09.0)

EEC	Eleva Examination Control Economy	
Weight	51 lbs	(24 kg)
Heat Dissipation	635 Btu/hr	(160 kcal/hr)

PHILIPS

Project
EasyDiagnost Eleva
Maine Medical Center
Portland, ME
- Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number:207-451-0546
Email: wayne.erwin@philips.com
Drawn By: JP Ganzhalian

Project Details
Drawing Number
N-EAS1006I12A
Date Drawn: 6/21/2010
Quote:1-PST1JCL Rev.7
Order:6900069926.001000

AD3

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or the utilities available at the premises on which the equipment is to be installed, used, or stored.

© Koninklijke Philips Electronics N.V. 2008. All rights reserved. Reproduction in whole or in part is prohibited without prior written consent of the copyright holder.

THIS SHEET IS PART OF THE DOCUMENT SET LISTED ON SHEET C1 AND SHOULD NOT BE SEPARATED.

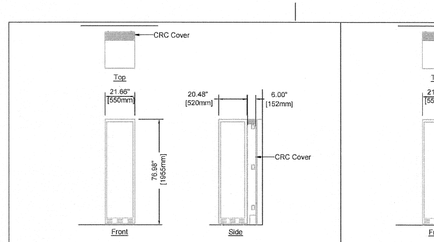

The CRC cover must be attached to the 40E rack only, not to the wall.

(08.0)

MR	EasyDiagnost R Rack	
Weight	213 lbs	(97 kg)
Heat Dissipation	1024 Btu/hr	(258 kcal/hr)

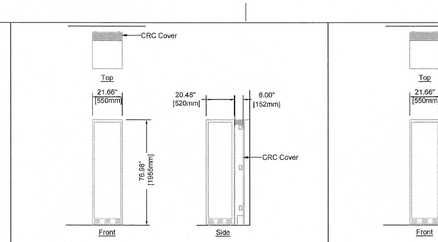

The CRC cover must be attached to the 40E rack only, not to the wall.

(08.0)

MB	Digital Imaging Control Cabinet	
Weight	454 lbs	(205 kg)
Heat Dissipation	3757 Btu/hr	(947 kcal/hr)

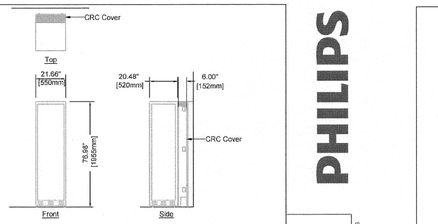

The CRC cover must be attached to the 40E rack only, not to the wall.

(08.0)

ME	Velara Generator Cabinet	
Weight	522 lbs	(237 kg)
Heat Dissipation	1706 Btu/hr	(430 kcal/hr)

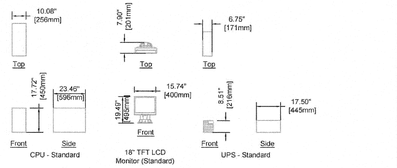

*** Total weight & BTU of standard equipment ***

(09.0)

VF	View Forum	
Weight	146 lbs**	(66 kg)
Heat Dissipation	1000 Btu/hr**	(252 kcal/hr)

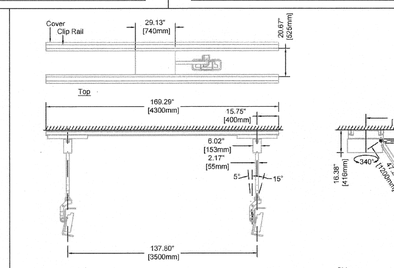

(10.0)

TV	One LCD Monitor Suspension (Hamburg)	
Weight	500 lbs	(226 kg)
Heat Dissipation	272 Btu/hr	(68 kcal/hr)

PHILIPS

Project
EasyDiagnost Eleva
Maine Medical Center
Portland, ME
- Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number:207-451-0546
Email: wayne.erwin@philips.com
Drawn By: JP Ganzhalian

Project Details
Drawing Number
N-EAS1006I12A
Date Drawn: 6/21/2010
Quote:1-PST1JCL Rev.7
Order:6900069926.001000

AD2

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or the utilities available at the premises on which the equipment is to be installed, used, or stored.

© Koninklijke Philips Electronics N.V. 2008. All rights reserved. Reproduction in whole or in part is prohibited without prior written consent of the copyright holder.

THIS SHEET IS PART OF THE DOCUMENT SET LISTED ON SHEET C1 AND SHOULD NOT BE SEPARATED.

EasyDiagnost Eleva Transport Information

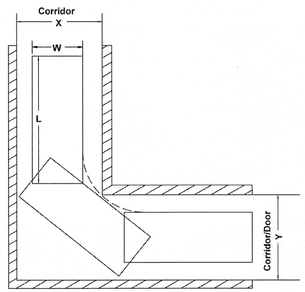

	Table Base		X-Ray Module		CS2
	Crate B Packed	Crate B Unpacked	Crate D Packed	Crate D Unpacked	Tube Support, Rails, and Carriage
Weight	718lbs (3195N)	651lbs (2895N)	1250lbs (5560N)	1025lbs (4560N)	966lbs (4300N)
Height	3'-11" (1.19m)	3'-8" (1.12m)	6'-8" (2.02m)	6'-4" (1.92m)	4'-8" (1.43m)
Length (L)	7'-2" (2.17m)	7'-2" (2.17m)	6'-0" (1.83m)	6'-0" (1.83m)	8'-0" (2.43m)
Width (W)	3'-8" (1.12m)	2'-6" (0.75m)	3'-1" (0.93m)	2'-9" (0.85m)	2'-8" (0.80m)

Width of Corridor "X"	Minimum Width of Corridor/Door "Y"		Minimum Width of Corridor/Door "Y"		Minimum Width of Corridor/Door "Y"
3'-4" (1.0m)	corridor X>W	5'-10" (1.78m)	6'-1" (1.84m)	5'-5" (1.66m)	6'-11" (2.10m)
3'-8" (1.1m)	corridor X>W	5'-5" (1.66m)	5'-4" (1.65m)	5'-0" (1.52m)	6'-5" (1.95m)
4'-0" (1.2m)	7'-2" (2.17m)	5'-1" (1.54m)	5'-0" (1.52m)	4'-7" (1.40m)	6'-0" (1.83m)
4'-4" (1.3m)	6'-6" (1.98m)	4'-9" (1.44m)	4'-8" (1.41m)	4'-3" (1.30m)	5'-8" (1.72m)
4'-8" (1.4m)	6'-1" (1.84m)	4'-5" (1.34m)	4'-4" (1.32m)	4'-0" (1.21m)	5'-4" (1.61m)
5'-0" (1.5m)	5'-7" (1.72m)	4'-1" (1.25m)	4'-1" (1.24m)	3'-9" (1.14m)	5'-0" (1.50m)
5'-3" (1.6m)	5'-4" (1.62m)	3'-10" (1.17m)	3'-10" (1.12m)	3'-6" (1.07m)	4'-8" (1.41m)
5'-7" (1.7m)	5'-0" (1.53m)	3'-7" (1.09m)	3'-8" (1.12m)	3'-4" (1.02m)	4'-4" (1.32m)
5'-11" (1.8m)	5'-5" (1.65m)	3'-4" (1.02m)	3'-7" (1.08m)	3'-3" (0.98m)	4'-1" (1.23m)
6'-3" (1.9m)	4'-6" (1.38m)	3'-2" (0.96m)	3'-5" (1.05m)	3'-2" (0.96m)	3'-10" (1.16m)
6'-7" (2.0m)	4'-4" (1.33m)	3'-0" (0.92m)	3'-5" (1.05m)	3'-1" (0.95m)	3'-8" (1.10m)

(08.0)

PHILIPS

Project
EasyDiagnost Eleva
Maine Medical Center
Portland, ME
- Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number:207-451-0546
Email: wayne.erwin@philips.com
Drawn By: JP Ganzhalian

Project Details
Drawing Number
N-EAS1006I12A
Date Drawn: 6/21/2010
Quote:1-PST1JCL Rev.7
Order:6900069926.001000

AD4

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or the utilities available at the premises on which the equipment is to be installed, used, or stored.

NOTE: THIS DRAWING WAS NOT PREPARED BY SMRT. IT IS PROVIDED FOR COORDINATION AND REFERENCE PURPOSES ONLY.

144 Fore Street/P.O. Box 618
Portland, Maine 04104
tel. (207) 772-3846
fax. (207) 772-1070
www.smrtinc.com

ARCHITECTURE
ENGINEERING
PLANNING
INTERIOR DESIGN
COMMISSIONING

SMRT

PROJECT NORTH

Bramhall Radiology
FLUORO RENOVATIONS
PORTLAND, ME

ISSUED FOR CONSTRUCTION
8.24.10

CURRENT ISSUE STATUS:

REV	DESCRIPTION	DATE
0	ISSUED FOR CONSTRUCTION	8.24.10

GRAPHIC SCALE: 0" 1"

SCALE:
PROJECT MANAGER: DJV
JC/DRAWN BY:
A/E OF RECORD: DJV
PROJECT NO: 09022-02
DATE: 8.24.10

SHEET TITLE:
VENDOR EQUIPMENT DRAWINGS SHEET 2

SHEET No.
Q- 002

©COPYRIGHT 2008 SMRT INC.