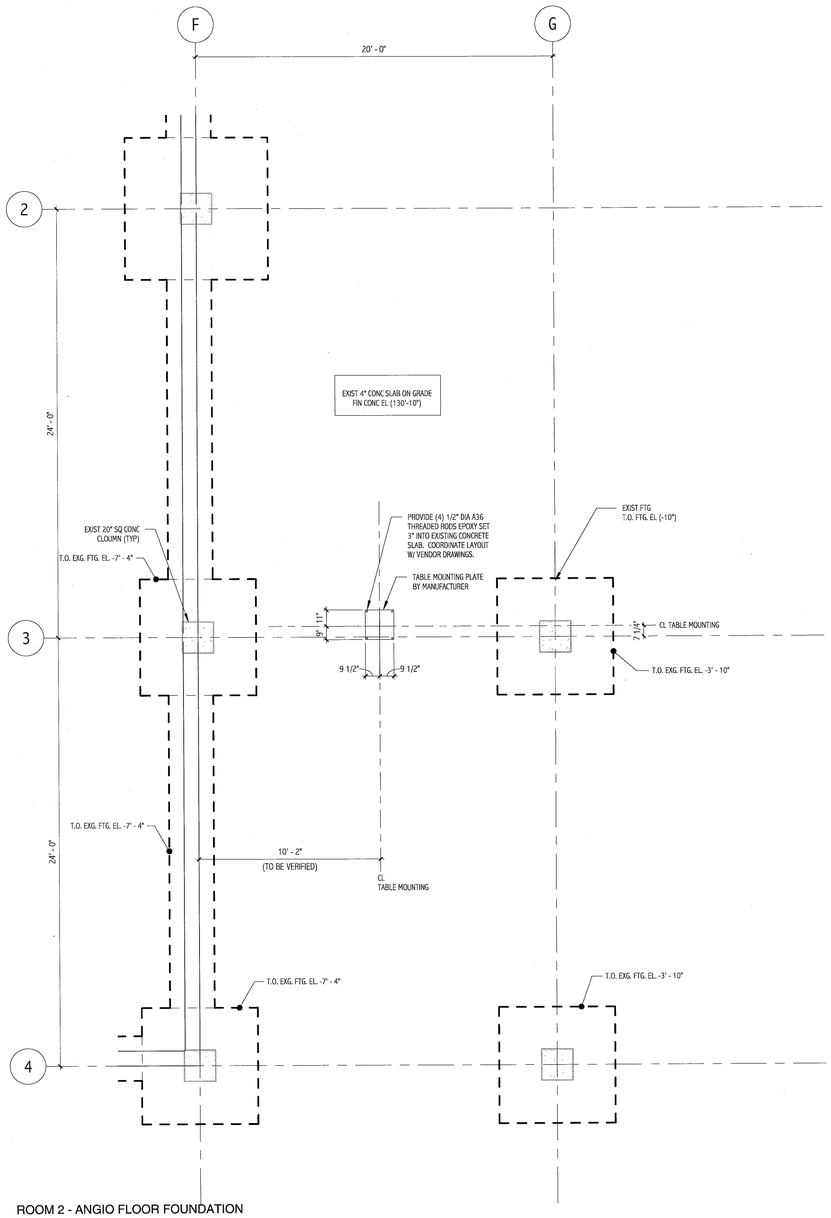

ROOM 2 - ANGIO FLOOR FOUNDATION PLAN
3 1/4" = 1'-0"

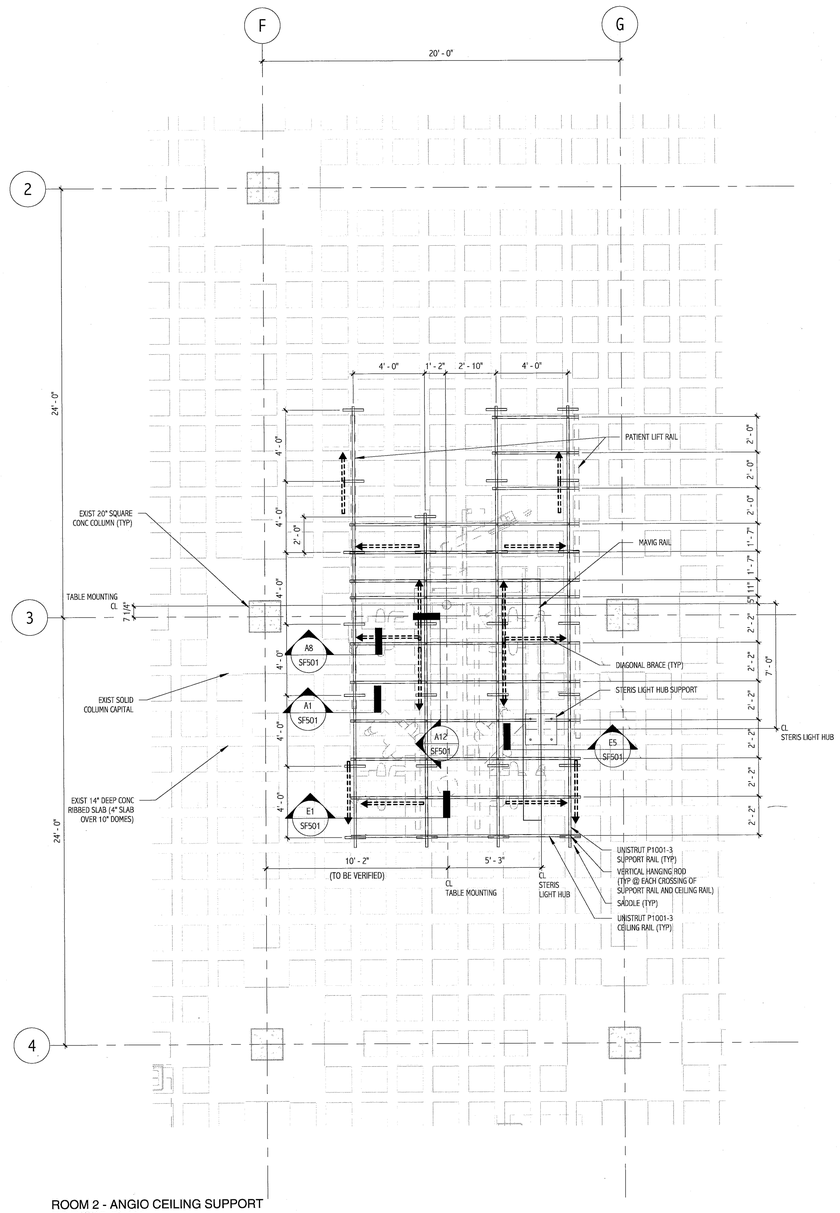

ROOM 2 - ANGIO CEILING SUPPORT FRAMING PLAN
2 1/4" = 1'-0"

NOTES:

1. STRUCTURAL SUPPORTS HAVE BEEN DESIGNED FOR THE FOLLOWING PIECES OF EQUIPMENT:
   A. SIEMENS ARTIS ZEE CEILING PER MANUFACTURER'S DRAWINGS DATED 1/3/2012.
   B. STERIS VLED 1 ARM LIGHT PER MANUFACTURER'S DRAWINGS DATED 11/21/2011.
   C. WAVERLY GLEN C SERIS PATIENT LIFT. FOLLOW MANUFACTURER'S GUIDELINES FOR X# TEST LOAD, RAIL SUPPORT DIMENSIONS X FT. SPANS AND X FT. CANTILEVER.
2. ITEMS NOTED AS "EPOXY SET" ARE TO BE USED WITH HILTI HIT-HY 150 MAX EPOXY.

144 Fore Street/P.O. Box 6418
Portland, Maine 04104
tel. (207) 772-3846
fax. (207) 772-1070
www.smrtinc.com

ARCHITECTURE
ENGINEERING
PLANNING
INTERIOR DESIGN
COMMISSIONING

SMRT

STATE OF MAINE
ANDREW D. BRADLEY
No. 9340
LICENSED
PROFESSIONAL ENGINEER

PROJECT NORTH
HUDSON/MAIN

MAINE MEDICAL CENTER
ANGIO SINGLE PLANE - ROOM 2
PORTLAND, ME

ISSUED FOR PERMITTING
01.27.12
CURRENT ISSUE STATUS

REV	DESCRIPTION	DATE

GRAPHIC SCALE:
0" 1"

SCALE:	As indicated
PROJECT MANAGER:	DW
IC/DRAWN BY:	SJF
A/E OF RECORD:	ADB
PROJECT NO:	11127
DATE:	XX.XX.XX

SHEET TITLE:
ANGIO FOUNDATION AND FRAMING PLANS

SHEET No.
SF101

©COPYRIGHT 2008 SMRT INC.