© Koninklijke Philips Electronics N.V. 2009. All rights reserved. Reproduction in whole or in part is prohibited without prior written consent of the copyright holder.

Equipment Closet
Site Specific

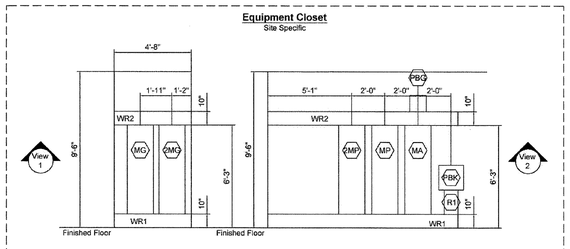

Control Room
Site Specific

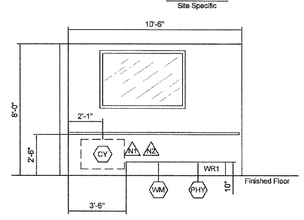

THIS SHEET IS PART OF THE DOCUMENT SET LISTED ON SHEET C1 AND SHOULD NOT BE SEPARATED

The use of 90 degree ells is not acceptable use 45 degree bends at all raceway corners. The use of crossover tunnels at all applicable locations is required.

* Countertop Height Guide:
30" for standard sealed height.
36" for standard standing height.
* Ensure that the wall junction boxes are mounted perpendicular to the floor.
* Verify exact ceiling height of Equipment and Control Room Area.

PHILIPS

Project
Allura Biplane FD10/10
Maine Medical Center
Portland, ME
Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number: (207) 651-0546
Email: wayne.erwin@philips.com
Drawn By: Jennifer Milka

Project Details
Drawing Number
N-EAS091441 F
Date Drawn: 8/5/2010
Quote: 1-FN8752 Rev. 11
Order:865001019791.001000

E2

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or of the utilities available at the premises in which the equipment is to be installed, used, or stored.

Conduit Required

General Notes

1. All conduit runs must take most direct route point to point.
2. All conduit runs must have a pull string.

A Conduit supplied/installed by contractor - Philips cables installed by Philips
B Conduit supplied/installed by contractor - Philips cables installed by contractor
C Conduits and cables supplied and installed by contractor
D Conduit existing - cables supplied and installed by Philips
E Conduit existing - cables supplied by Philips, installed by contractor
F Conduit existing - cables supplied and installed by contractor
G Optional equipment, verify with local Philips Service

P Power (AC)
D Power (DC)
G Ground
S Signal
H High Tension
C Cooling Hose
A Air Supply Hose

	Run No.	Conduit From	Conduit To	Conduit Quantity	Cable Type (*)	Minimum Conduit Size	Maximum Conduit Length	Special Requirements
C	1	Power Panel	CB	1	(P)	Per N.E.C.	Per N.E.C.	
B	2	PBK	PDU Cabinet	1	(P)	1 1/2"	-	
B	3	PBK	PDU Cabinet	2	(P)	2"	-	
B	4	CB	PBK	1	(P)	2"	50'	
C	5	CB	ST	1	(P)	3/4"	50'	
C	6	PBK	GE	1	(P)	3/4"	25'	
C	7	PBG	Room Outlets	1	(P)	3/4"	-	See Sheet "ED2" for details.
C	8	MA	WL	1	(P)	3/4"	55'	
C	9	ATY	DS	1	(S)	3/4"	55'	
A	10	SP	MG	1	(H)	2 1/2"	44'	H.T. Cables.
A	11	SP	MG	1	(P)	1"	44'	
A	12	SP	MG	1	(S)	1 1/2"	44'	
A	13	SP	MP	1	(S)	2 1/2"	49'	
A	14	SP	MP	1	(P)	1"	49'	
A	15	SP	MP	2	(C)	2"	49'	Cooling fluid hoses for tube.
A	16	SP	MP	2	(C)	2 1/2"	49'	Cooling fluid hoses for detector.
A	17	SP	MA	1	(S)	2 1/2"	50'	
A	18	MSA	MP	1	(S)	2 1/2"	49'	
A	19	MSA	MP	1	(P)	1"	49'	
A	20	MSA	MA	1	(S)	2 1/2"	49'	
A	21	MSA	MA	1	(P)	3/4"	49'	
C	22	MP	Stub	1	(S)	1"	-	Stub above finished ceiling. Recommended for possible future network connection if desired by customer.
G	23	MP	HCU	1	(S)	3"	90'	Not needed if HCU is connected via network.
G	24	PHY	MSA	1	(S)	2 1/2"	-	
G	25	PHY	Physio Monitor	1	(S)	2"	33'	Optional for remote location.
A	26	TV	MA	1	(P)	2"	52'	
A	27	TV	MA	1	(S)	2 1/2"	52'	
A	28	TV	MP	1	(S)	1 1/2"	54'	
A	29	ATY	MA	1	(S)	2 1/2"	41'	
A	30	ATY	TV	1	(S)	3/4"	75'	

Conduit Required

General Notes

1. All conduit runs must take most direct route point to point.
2. All conduit runs must have a pull string.

A Conduit supplied/installed by contractor - Philips cables installed by Philips
B Conduit supplied/installed by contractor - Philips cables installed by contractor
C Conduits and cables supplied and installed by contractor
D Conduit existing - cables supplied and installed by Philips
E Conduit existing - cables supplied by Philips, installed by contractor
F Conduit existing - cables supplied and installed by contractor
G Optional equipment, verify with local Philips Service

P Power (AC)
D Power (DC)
G Ground
S Signal
H High Tension
C Cooling Hose
A Air Supply Hose

	Run No.	Conduit From	Conduit To	Conduit Quantity	Cable Type (*)	Minimum Conduit Size	Maximum Conduit Length	Special Requirements
A	31	CY	MP	1	(S)	2"	50'	
A	32	CY	MA	1	(P)	2"	55'	
A	33	CY	MA	1	(S)	2 1/2"	55'	
A	34	CY	CMP	1	(S)	3/4"	55'	
A	35	MA	WM	1	(S)	1"	82'	
A	36	PB1	CMC	1	(H)	2 1/2"	44'	H.T. Cables.
A	37	PB1	CMC	1	(P)	1"	44'	
A	38	PB1	CMC	1	(S)	1 1/2"	44'	
A	39	PB1	CMP	2	(C)	2"	50'	Cooling fluid hoses for tube.
A	40	PB1	MP	2	(C)	2 1/2"	41'	Cooling fluid hoses for detector.
A	41	PB1	MP	1	(S)	2 1/2"	41'	
A	42	PB1	MP	1	(S)	1"	41'	
A	43	PB1	MA	1	(S)	2"	41'	
G	44	TV	Control Room	2	(S)	1 1/2"	-	Verify with local Philips Service (Physio Monitor).
G	45	TV	Control Room	2	(S)	1 1/2"	-	For optional equipment (Interventional Hardware, ViewForum. Xcelera. etc). For future options (Bolus Chase, 3D-RA and Tableside Analysis Module).
G	46	MSA	Control Room	2	(S)	1 1/2"	-	
C	47	Power Panel	CB2	1	(P)	2"	-	Do not duplicate for each lab (See Sheet "ED4").
C	48	CB2	UPS	1	(P)	1 1/2"	-	Do not duplicate for each lab (See Sheet "ED4").
C	49	UPS	CB3	1	(P)	1 1/2"	-	
C	50	PBK	UTS	1	(P)	2"	75'	
C	51	UTS	CMC	1	(P)	2"	75'	
C	52	UTS	CMC	1	(P)	1"	75'	
C	53	UTS	MG	1	(P)	2"	75'	
C	54	UTS	MG	1	(P)	1"	75'	
C	55	UTS	MA	1	(P)	1"	75'	
C	56	UTS	MA	1	(P)	3/4"	75'	
C	57	CB2	UTS	1	(P)	1 1/2"	150'	
C	58	CB3	ST	1	(P)	3/4"	150'	
C	59	BC	UPS	1	(P)	2"	-	Do not duplicate for each lab (See Sheet "ED4").
G	60	RSM	UPS	1	(P)	1 1/2"	250'	Remote Status Monitor (Optional).

PHILIPS

Project
Allura Biplane FD10/10
Maine Medical Center
Portland, ME
Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number: (207) 651-0546
Email: wayne.erwin@philips.com
Drawn By: Jennifer Milka

Project Details
Drawing Number
N-EAS091441 F
Date Drawn: 8/5/2010
Quote: 1-FN8752 Rev. 11
Order:865001019791.001000

E3

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or of the utilities available at the premises in which the equipment is to be installed, used, or stored.

Conduit Required

General Notes

1. All conduit runs must take most direct route point to point.
2. All conduit runs must have a pull string.

A Conduit supplied/installed by contractor - Philips cables installed by Philips
B Conduit supplied/installed by contractor - Philips cables installed by contractor
C Conduits and cables supplied and installed by contractor
D Conduit existing - cables supplied and installed by Philips
E Conduit existing - cables supplied by Philips, installed by contractor
F Conduit existing - cables supplied and installed by contractor
G Optional equipment, verify with local Philips Service

P Power (AC)
D Power (DC)
G Ground
S Signal
H High Tension
C Cooling Hose
A Air Supply Hose

	Run No.	Conduit From	Conduit To	Conduit Quantity	Cable Type (*)	Minimum Conduit Size	Maximum Conduit Length	Special Requirements

Conduit Required

General Notes

1. All conduit runs must take most direct route point to point.
2. All conduit runs must have a pull string.

A Conduit supplied/installed by contractor - Philips cables installed by Philips
B Conduit supplied/installed by contractor - Philips cables installed by contractor
C Conduits and cables supplied and installed by contractor
D Conduit existing - cables supplied and installed by Philips
E Conduit existing - cables supplied by Philips, installed by contractor
F Conduit existing - cables supplied and installed by contractor
G Optional equipment, verify with local Philips Service

P Power (AC)
D Power (DC)
G Ground
S Signal
H High Tension
C Cooling Hose
A Air Supply Hose

	Run No.	Conduit From	Conduit To	Conduit Quantity	Cable Type (*)	Minimum Conduit Size	Maximum Conduit Length	Special Requirements

PHILIPS

Project
Allura Biplane FD10/10
Maine Medical Center
Portland, ME
Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number: (207) 651-0546
Email: wayne.erwin@philips.com
Drawn By: Jennifer Milka

Project Details
Drawing Number
N-EAS091441 F
Date Drawn: 8/5/2010
Quote: 1-FN8752 Rev. 11
Order:865001019791.001000

E4

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or of the utilities available at the premises in which the equipment is to be installed, used, or stored.

Detail - PDU 4000 Mounting Detail



PDU 4000 with J-box "PBK" flush or surface mounted behind unit.

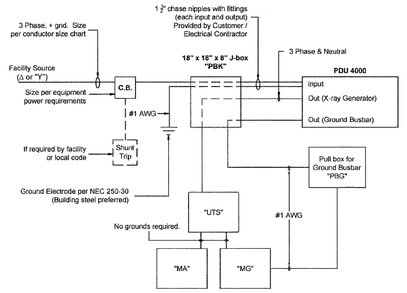

Note: Conductors, destinations, and number of conduit runs from PDU to J-box "PBK" and from J-box to equipment will vary from system to system. Consult individual site plans for detailed conduit schedules.

Diagram - PDU 4000 Electrical Interface with UTS (08.0)

PBK

Power Quality Requirements
Velara 100KW with PDU 4000

Power Output:	100KW
Supply Configuration:	3 phase, 3 wire power and ground, Delta or wye 3 phase, 4 wire power w/ Neutral + ground, wye
Nominal Line Voltage:	480 VAC, 60 Hz
Line Voltage Variation:	± 10% steady-state
Line Voltage Balance:	2% maximum of nominal voltage between phases
Frequency Variation:	± 1.0 Hz
Voltage Surges:	To 110% of steady-state voltage 100 msecs. Maximum duration, 6 per hour maximum
Voltage Sags:	To 90% of steady-state voltage 100 msecs. Maximum duration, 6 per hour maximum
Line Impulses:	1000 VPK above phase-neutral RMS absolute maximum. No more than 1 impulse per hour to exceed 500 VPK.
Neutral-Ground Voltage:	2.0 volts maximum RMS value
Neutral-Ground Impulses:	No more than 1 per hour that exceeds 25 volts and 1 Mjoule
High Frequency Noise:	3.0 volts steady-state maximum. Over 3.0 volts permitted for 100 msec. maximum, 1 per hour max.
Grounded Conductor Impedance:	0.1 Ohms @ 60 hz. maximum

Branch Circuit and Wire Gauge Requirements
Velara 100KW with PDU 4000

Branch Power:	225 KVA
Max Stand by Current:	8 Amps. @ 3 mA, 110 KVP continuous
Circuit Breaker:	3 pole, 125 amperes
Maximum Instantaneous Power:	201 KVA (1000 mA @ 100 KVP)

Recommended conductor sizes for 1% impedance of branch conductors to circuit breaker (CB). Based on 20° copper conductors:

	480VAC
1/0 AWG	95ft
2/0 AWG	120ft
3/0 AWG	151ft
4/0 AWG	193ft
250 KCM	226ft
300 KCM	271ft
400 KCM	365ft
Inst. Current @ CB Panel	242 A
Max. Phase-phase impedance @ CB Panel	≤ 200 mΩ
Max. Load Voltage Drop @ CB Panel	18.2 V
Percent Regulation at Maximum Load @ CB Panel	3.8%
Output Voltage PDU 4000:	480 VAC ± 10%
Max Inst. Current @ PDU output:	305 Amps
Max Phase-Phase Impedance:	≤ 200 mΩ @ PDU output
Max Load Voltage Drop:	24.4 V @ PDU output
Percent Regulation at Max. Load:	6.4% @ PDU output

Minimum copper wire size, circuit breaker to PDU: #1 - Maximum 50' in length.

CB

PHILIPS

Project
Allura Biplane FD10/10
Maine Medical Center
Portland, ME
Room 5

Philips Contacts
Project Manager: Wayne Erwin
Contact Number: (207) 651-0546
Email: wayne.erwin@philips.com
Drawn By: Jennifer Milka

Project Details
Drawing Number
N-EAS091441 F
Date Drawn: 8/5/2010
Quote: 1-FN8752 Rev. 11
Order:865001019791.001000

ED1

THE INFORMATION IN THIS PACKAGE IS PROVIDED AS A CUSTOMER CONVENIENCE, AND IS NOT TO BE CONSTRUED AS ARCHITECTURAL DRAWINGS OR CONSTRUCTION DOCUMENTS. Philips assumes no liability nor offers any warranty for the fitness or adequacy of the premises or of the utilities available at the premises in which the equipment is to be installed, used, or stored.

THIS SHEET IS PART OF THE DOCUMENT SET LISTED ON SHEET C1 AND SHOULD NOT BE SEPARATED.

NOTE: THIS DRAWING WAS NOT PREPARED BY SMRT. IT IS PROVIDED FOR COORDINATION AND REFERENCE PURPOSES ONLY

144 Fore Street/P.O. Box 618
Portland, Maine 04104
tel. (207) 772-3846
fax. (207) 772-1070
www.smrtinc.com

ARCHITECTURE ENGINEERING PLANNING INTERIOR DESIGN COMMISSIONING

SMRT

PROJECT NORTH

MAIN ENTRY

MAINE MEDICAL CENTER CATH. LAB #5
PORTLAND, ME

ISSUED FOR CONSTRUCTION
9.3.10

CURRENT ISSUE STATUS:

REV	DESCRIPTION	DATE
0	ISSUED FOR CONSTRUCTION	9.3.10

GRAPHIC SCALE: 0" 1"

SCALE:
PROJECT MANAGER: KD
JC/DRAWN BY:
A/E OF RECORD:
PROJECT NO: 10006-00
DATE: 9.3.10

SHEET TITLE:
VENDOR EQUIPMENT DRAWINGS, SHEET 6

SHEET No.
Q-006

©COPYRIGHT 2009 SMRT INC.